

Original article

In vitro biocompatibility of novel titanium-based amorphous alloy thin film in human osteoblast like cells

Saran Tantavisut^a, Boonrat Lohwongwatana^b, Atchara Khamkongkao^b, Aree Tanavalee^a, Pairat Tangpornprasert^c, Pubul Ittiravivong^a

^aDepartment of Orthopaedic, Faculty of Medicine, Chulalongkorn University

^bDepartment of Metallurgical Engineering, Faculty of Engineering, Chulalongkorn University

^cDepartment of Mechanical Engineering, Faculty of Engineering, Chulalongkorn University

Background: Toxic free Ti-based amorphous alloy has potential to be used in biomedical fields due to its excellent biocompatibility and nontoxic elements such as Al, Ni, V and Be.

Objectives: The purpose of this study was to develop a series of Ti₄₄Zr₁₀Pd₁₀Cu_{6+x}Co_{23-x}Ta₇ (x = 0, 4, 8) and examine their biocompatibility, biological property, and toxicity in osteoblast like cells.

Methods: Having developed the alloy ingots by induction melting technique, we used the cast rod as plasma cathode in filtered cathodic vacuum arc deposition chamber to coat a 25-nm thin film amorphous alloy on cover glass slides. These coated cover glass slides were then examined for biocompatibility. The biocompatibility tests in SaOS2 osteoblast like cells were performed using methylthiazol tetrazolium assay and alizarin red staining. The medical grade Ti-6Al-4V alloys was studied in parallel as a control material.

Results: There was no statistically significant difference in number of living cells between all novel alloys compared with Ti-6Al-4V thin film. Alizarin red staining assay showed that all novel alloy thin film had significantly higher percentage area of calcification in comparison with Ti-6Al-4V thin film control (P < 0.05). In term of calcification size, the Ti₄₄Zr₁₀Pd₁₀Cu₁₀Co₁₉Ta₇ and Ti₄₄Zr₁₀Pd₁₀Cu₁₄Co₁₅Ta₇ showed significantly greater calcification than control (P < 0.05) while Ti₄₄Zr₁₀Pd₁₀Cu₆Co₂₃Ta₇ also demonstrated larger calcification in comparison with control but no statistical significance (P = 0.27).

Conclusion: The results indicated that all investigated Ti-based alloys were found to be non-cytotoxic and support differentiation of osteoblast-like cells.

Keywords: Titanium-based alloy, biocompatibility, toxicity, calcification.

Amorphous alloys or metallic glass is a new class of alloys which has gained wide attention due to their superior properties compared with the conventional crystalline alloys. Metallic glass formation is achieved by passing nucleation and growth of crystalline phases when the alloy is rapidly cooled from the molten liquid. ⁽¹⁾ In general, metallic glass has superior strength, lower elastic modulus, better corrosion resistance, better wear resistance and unique processing capabilities comparing with crystalline alloy

counterparts. The unique properties of amorphous alloys have a potential to solve problems encountered by traditional orthopedic implant materials. ^(2, 3) Ti-based amorphous alloy is one of the most popular alloy because of its potential to be used as biomaterial. However, many of the Ti-based amorphous alloys contains toxic element including Al, Ni, V and Be. These toxic elements can be released from the alloys and causes long-term health problem, for example, peripheral neuropathy, osteomalacia and Alzheimer's diseases. ^(4, 5) We tried to obtained better performance and safer material of the Ti-base amorphous alloy by exploring new compositions. This study was aimed to develop a novel biocompatible composition, toxic-free Ti-based amorphous alloy and to study *in vitro* biocompatibility of this novel alloy using Ti-6Al-4V alloy as a reference material in human osteoblast

Correspondence to: Lohwongwatana B. Department of Metallurgical Engineering, Faculty of Engineering, Chulalongkorn University, Bangkok, 10330, Thailand.

Received : January 26, 2018

Revised : July 24, 2018

Accepted: September 25, 2018

like cells. The microscopic methodology was used to examine the biocompatibility and alloy characterization.

Materials and Methods

Ti-based alloy ingots with a nominal composition of $\text{Ti}_{44}\text{Zr}_{10}\text{Pd}_{10}\text{Cu}_{6+x}\text{Co}_{23-x}\text{Ta}_7$ ($x = 0, 4, 8$) were synthesized using arc-melting 6 elements of 99.9% or higher purity in a titanium-gettered argon atmosphere. Ti-6Al-4V alloy was used as a reference material. Cylindrical rod samples with a diameter of 5 mm and length of 20 mm were fabricated by copper mold casting technique. The cylindrical rods of 3 new alloy formula and Ti-6Al-4V as a reference material were then used as plasma cathode in filtered cathodic vacuum arc (FCVA) deposition technique to make Ti-based thin film metallic glass which is coated on around glass substrate with a diameter 1.5 cm. The Ti-based thin film on glass substrate was further employed for biocompatibility tests.

We performed biocompatibility test in human osteoblast-like cells (SaOS2) *in vitro*. Before every test, the coated discs were sterilized by autoclaving. A human osteoblast-like cell line (SaOS-2), were used for biocompatibility test in the present study. SaOS-2 cells were cultured in Dulbecco's modified Eagle's medium (DMEM). The medium was supplemented with 10% fetal bovine serum, 2mM L-glutamine, 100 unit/ml penicillin, 100 $\mu\text{g}/\text{ml}$ Streptomycin and 0.25 $\mu\text{g}/\text{ml}$ amphotericin B. Cells were maintained at 37°C in 100% humidity and 5% CO_2 . Confluent cells were detached using 0.25% trypsin with ethylene diamine tetraacetic acid and re-suspended in fresh culture medium. The media were changed every 2-3 days. Cell proliferation was determined by methylthiazol tetrazolium (MTT) assay. Cells were seeded on triplicate samples discs ($n = 3$) with a concentration of 50,000 cells/well in a 24-well plate. The assay was performed on day 3. After completing the culture period, the media was gently removed and the specimens were rinsed with phosphate-buffered saline (PBS) to remove unattached cells and to avoid the effects of media on the biochemical assays. Then MTT solution (300 μL ; 0.5 mg/mL 3-(4, 5-Dimethylthiazol-2-yl)-2, 5-diphenyltetrazolium bromide in culture medium without phenol red) was added. After 30 minutes of incubation, MTT solution was discarded and then formazan crystals were dissolved in dimethylsulfoxide (DMSO) (900 $\mu\text{L}/\text{well}$) and

glycine buffer (pH = 10) (125 $\mu\text{L}/\text{well}$). The absorbance was read at a wavelength of 570 nm by Thermospectronic Genesis 10 UV-vis spectrometer.

Alizarin is an organic compound that could react with calcium ions. Alizarin red S, a dye that stains calcium salts selectively and is widely used for mineral histochemistry of calcium, served to analyze the mineralization level of cells. In this study, SaOS2 1.0×10^5 cells were seeded onto the disc. The osteogenic inductions were induced after 24 hours. On day 28, the medium was discarded then the cells on the discs were fixed with 95% ethanol for 10 minutes, and then rinsed several times with distilled water; 0.1% Alizarin red was added onto the disc then incubated at 37°C for 30 minutes and rinsed several times with distilled water before being proceeded to light microscope evaluation under 10x magnification.

Results

The SaOS2 cell proliferation was determined by MTT assay on day 3 are shown in Figure 1. There was no statistically significant difference in number of living cells between all the novel alloys compared with thin film Ti-6Al-4V. Alizarin red staining in Ti-6Al-4V and novel metallic glass alloys, the results were shown in Figure 2. Alizarin red staining assay showed that all novel alloy thin film had significantly higher percentage area of calcification compared with Ti-6Al-4V thin film control ($P < 0.05$). In term of calcification size, the $\text{Ti}_{44}\text{Zr}_{10}\text{Pd}_{10}\text{Cu}_{10}\text{Co}_{19}\text{Ta}_7$ and $\text{Ti}_{44}\text{Zr}_{10}\text{Pd}_{10}\text{Cu}_{14}\text{Co}_{15}\text{Ta}_7$ showed significantly greater calcification than control ($P < 0.05$) while $\text{Ti}_{44}\text{Zr}_{10}\text{Pd}_{10}\text{Cu}_{6}\text{Co}_{23}\text{Ta}_7$ also demonstrated larger calcification compared with control but no statistical significance ($P = 0.27$).

Alizarin red staining assay was analyzed using Image J program (set color threshold as RGB: 200, 120, 80) to quantify the calcium mineralization. The results were demonstrated in Table 1. Alizarin red staining assay showed that all novel alloy thin film had significantly more % area of calcification compared with Ti-6Al-4V thin film control (all $P < 0.05$). In term of calcification size, the $\text{Ti}_{44}\text{Zr}_{10}\text{Pd}_{10}\text{Cu}_{10}\text{Co}_{19}\text{Ta}_7$ and $\text{Ti}_{44}\text{Zr}_{10}\text{Pd}_{10}\text{Cu}_{14}\text{Co}_{15}\text{Ta}_7$ showed significantly greater calcification (both had $P < 0.05$) while $\text{Ti}_{44}\text{Zr}_{10}\text{Pd}_{10}\text{Cu}_{6}\text{Co}_{23}\text{Ta}_7$ also demonstrated bigger calcification compared with control but no statistical significance ($P = 0.27$).

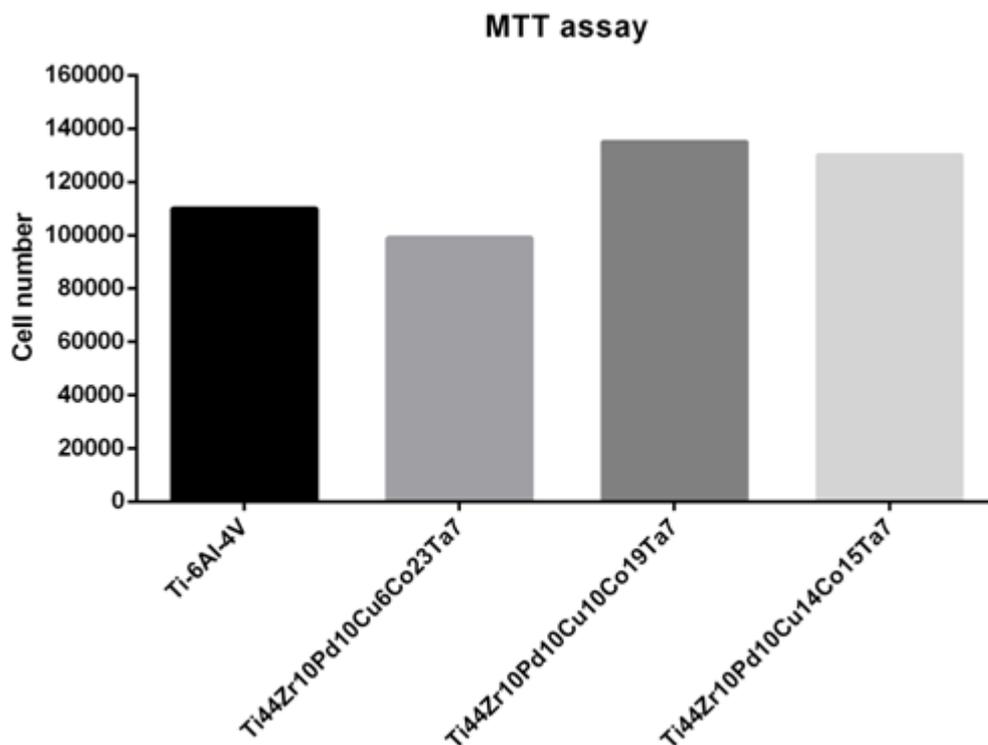


Figure 1. MTT assay of SaOS2 cells on Ti-6Al-4V and the series of novel Ti-based MG thin film.

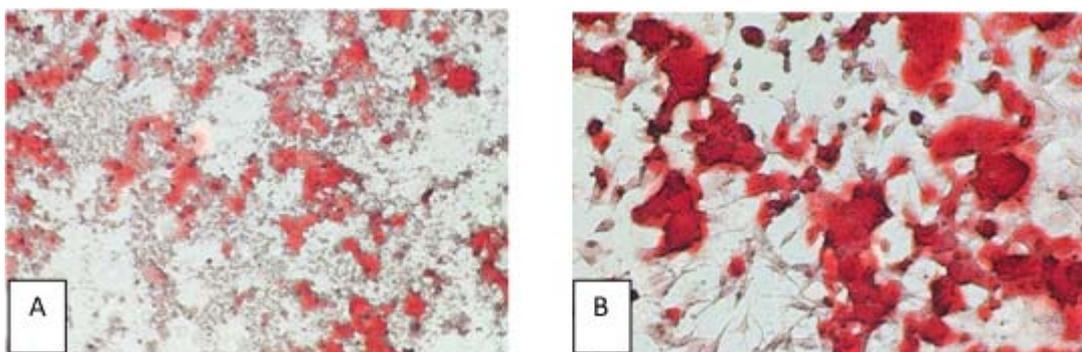


Figure 2. The Alizarin red staining results of SaOS2 cells on Ti-6Al-4V (Figure 2A) and the novel Ti₄₄Zr₁₀Pd₁₀-Cu₁₄Co₁₅Ta₇ thin film (Figure 2B).

Table 1. Quantitative analysis of Alizarin red staining using Image J program.

	Ti ₆ Al ₄ V	Ti ₄₄ Zr ₁₀ Pd ₁₀ - Cu ₆ Co ₂₃ Ta ₇	Ti ₄₄ Zr ₁₀ Pd ₁₀ - Cu ₁₀ Co ₁₉ Ta ₇	Ti ₄₄ Zr ₁₀ Pd ₁₀ - Cu ₁₄ Co ₁₅ Ta ₇
% Area	4.3%	7.1%	9.8%	18.6%
Average size (pixels)	96.3 ± 18.6	103.7 ± 5.3	310.5 ± 27.6	398.9 ± 106.5

Discussion

In the previous report, the new Ti-based alloy composite without toxic elements has been synthesized in TiZrCuPd alloy system such as Ti₄₀Zr₁₀Cu₃₆Pd₁₄, which exhibit high corrosion resistance and good combination of strength and ductility, implying a high potential as biomaterials.⁽⁶⁾ We developed our metallic glass based on this combination. We decided to decrease Copper composition due to the reported cytotoxicity of Cu to 3T3 fibroblast cell line tests.⁽⁷⁾ Copper containing crystalline alloy and amorphous alloy have been reported about cell toxicity. Elshahawy WM, *et al.*⁽⁸⁾ stated that Cu released from gold alloys which are commonly used as fixed prosthodontic restorations, show evidence of a high cytotoxic effect on fibroblast cells. In contrast, recent study did not demonstrated negative effects of copper containing alloys to the cells⁽⁹⁾ and there were compatible with results of our study. The explanation of this issue is the formation of TiO₂ that developed on the surface of novel Ti based alloy which contain Ti 44 atomic percentage. The TiO₂ has been reported about ability to provide good biocompatibility and bactericidal effect.⁽¹⁰⁾ It may conceal the copper from direct contact to the cells or decrease the copper ion release into the cell growth medium to the optimum level. In addition, our novel alloy compositions contain lower amount of copper than the alloy previously reported then may lead to less toxicity from copper. The results in our experiment are compatible with many previous published articles which focused on toxic free amorphous alloy containing copper composition. Qin FX, *et al.*⁽¹¹⁾ have developed amorphous alloy with component of Ti₄₀Zr₁₀Cu_{40- \times} Pd_{10+ \times} (with $\times = 0, 2, 4, 6, 8$ and 10). They reported good mechanical property and good biocompatibility of their series of amorphous alloy. Oak JJ, *et al.* conducted human osteoblast like cells SAOS2 on Ti₄₅Zr₁₀Pd₁₀Cu₃₁Sn₄ and found results of good biocompatibility and glass forming ability.⁽¹²⁻¹³⁾ However, due to the nature of novel material, it is impossible to find a previously matched amorphous alloy to study in comparison with the current study results. In our study, after the cells were exposed to all the novel amorphous alloy samples for 3 days, there was no significant difference in cell proliferation and differentiation compared to the glass substrate and Ti-6Al-4V control, suggesting that Ti-based MG thin film was non-toxic to SaOS2.

Conclusion

The novel Ti-based amorphous alloy Ti₄₄Zr₁₀Pd₁₀Cu_{6+ \times} Co_{23- \times} Ta₇ ($\times = 0, 4, 8$) demonstrated biocompatible characteristics to osteoblast like-cells (SaOS2). These results suggest that the novel Ti-based amorphous alloy may be applied to potentially develop for using as biomedical applications.

Conflict of interest

None of the authors has any potential conflict of interest to disclose.

References

1. Inoue A, Wang XM, Zhang W. Developments and applications of bulk metallic glasses. *Rev Adv Mater Sci* 2008;18:1-9.
2. Schroers J, Kumar G, Hodges TM, Chan S, Kyriakides TR. Bulk metallic glasses for biomedical applications. *JOM* 2009;61:21-29.
3. Schuh CA, Hufnagel TC, Ramamurty U. Mechanical behavior of amorphous alloys. *Acta Materialia* 2007; 55:4067-109.
4. Rao S, Uchida T, Tateishi T, Okazaki T, Asao Y. Effects of Ti, Al and V ions on the relative growth rate of fibroblasts (L929) and osteoblasts (MC3T3-E1) cells. *J Biomed Mater Eng* 1996;6:79-86.
5. Walker PR, Leblanc J, Sikorska M. Effects of aluminium and other cations on the structure of brain and liver chromatin. *Biochemistry* 1989;28:3911-5.
6. Qin FX, Wang XM, Inoue A. Effect of annealing on microstructure and mechanical property of a Ti-Zr-Cu-Pd bulk metallic glass. *Intermetallics* 2007;15: 1337-42.
7. Buzzi S, Jin K, Uggowitz PJ, Tosatti S, Gerber I, Loffler JF. Cytotoxicity of Zr-based bulk metallic glasses. *Intermetallics* 2006;14:729-34.
8. Elshahawy WM, Watanabe I, Kramerb P. In vitro cytotoxicity evaluation of elemental ions released from different prosthodontic materials. *Dent Mater* 2009;25:1551-5.
9. Zhu SL, Wang XM, Inoue A. Glass-forming ability and mechanical properties of Ti-based bulk glassy alloys with large diameters of up to 1 cm. *Intermetallics* 2008;16:1031-5.
10. Visai L, Nardo LD, Punta C, Melone L, Cigada A, Imbriani M, et al. Titanium oxide antibacterial surfaces in biomedical device. *Int J Artif Organs* 2011;34: 929-46.
11. Qin FX, Wang XM, Inoue A. Effects of Ta on Microstructure and Mechanical Property of Ti-Zr-Cu-

- Pd-Ta Alloys. *Mater Trans* 2007;48:2390-4.
12. Oak JJ, Louzguine-Luzgin DV, Inoue A. Investigation of glass forming ability, deformation and corrosion behavior of Ni free Ti-based BMG alloys designed for application as dental implant. *Mater Sci Eng A* 2009;29:322-7.
 13. Oak JJ, Hwang GW, Park YH, Kimura H, Yoon SY, Inoue A. Characterization of surface properties, osteoblast cell culture in Vitro and processing with flow viscosity of Ni free Ti-based bulk metallic glass for biomaterials. *J Biomech Sci Eng* 2009;4:384-91.